

Vitreoretinal Product Catalog

www.fciworldwide.com





FCI S.A.S. is a world leader in the development of a wide range of ophthalmic surgical devices.

Since the company's inception in 1984, the innovative developments of FCI have helped physicians to solve problems related to epiphora, dry eye, eyelids, and orbital surgery as well as retinal detachment : highly purified silicone oil and perfluorocarbons, scleral buckling implants, and a wide range of other ophthalmic surgical devices such as disposable vitrectomy lenses, single use instruments and directional laser probes.

FCI performs extensive research and development to provide physicians with outstanding products that enhance the efficiency and effectiveness of retinal procedures.

This line of product is FCI latest commitment to provide you with high performance products in retinal surgery.





TABLE OF CONTENTS

MEDICAL RETINA

INTRAVITREAL INJECTION ASSISTANT	4
<i>Precivia®</i>	
INTRAVITREAL INJECTION KIT	5
<i>Precivia® Pack</i>	

SURGICAL RETINA

ENDO-PROBES	6
<i>90° Adjustable laser probes, Directional laser probe, Laser probes, Laser illumination probes, Light probes</i>	
OPHTHALMIC SURGICAL LIQUIDS	16
<i>Purified silicone oil, RetiJet®, PFCL</i>	
SCLERAL BUCKLES	19
<i>ePTFE, Silicone (bands, strips, tires, fixation sleeves, cords, sponges),</i>	
ACCESSORIES	24
<i>Trocars, Disposable backflush with T-tube, Cannulas, Disposable vitrectomy lenses, FCI Protect® - 2.0% HPMC, Disposable three mirror lens, Iris retractors</i>	
VITREORETINAL INSTRUMENTS	30
<i>Single use instruments</i>	

PRECIVIA® PRECISION INTRAVITREAL INJECTION ASSISTANT

Precivia® is a disposable device that simplifies* intravitreal injections. Its special design ensures a fast, accurate & predictable procedure*.

**FCI
EXCLUSIVE**

Eliminates unnecessary instruments

- No speculum, caliper or pressure plate needed.

Assures accuracy


- Fixed guide ensures proper angle, depth & distance of injection every time.

Relaxes patients*

- Precivia® immobilizes the eye & hides the needle resulting in less patient anxiety.

Prevents leakage*

- Rotating the device pre & post injection, displaces & replaces the conjunctiva over the injection hole.

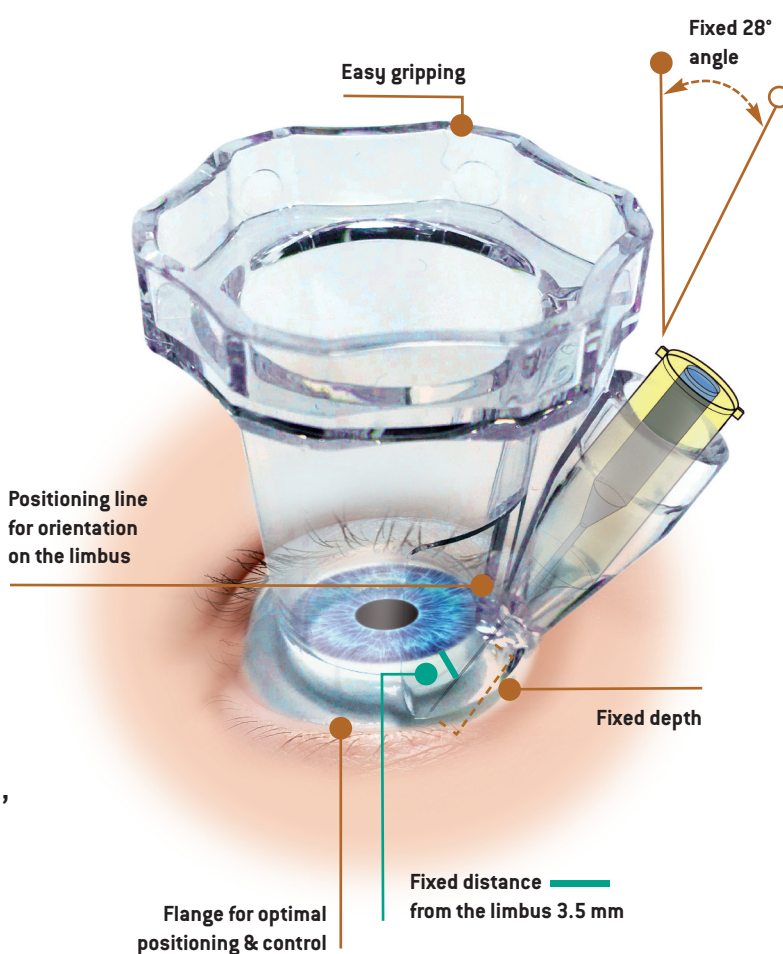

*References: Ratnarajan G, Nath R, Appaswamy S, et al. Intravitreal injections using a novel conjunctival mould: a comparison with a conventional technique. British Journal of Ophthalmology 2013;97:395-397. Petri, A., Boysen, K., Cehofski, L.J. et al. Intravitreal Injections with Vascular Endothelial Growth Factor Inhibitors: A Practical Approach. Ophthalmol Ther 9, 191–203 (2020).

PRECIVIA®

FOR LUCENTIS®₁ & EYLEA®₂

- For Lucentis® injection: prefilled syringe & vial format
- For Eylea® injection: vial format
- Compatible with BD 30 Ga 13 mm cannula & B/Braun Lucentis® Sterican® 30 Ga cannula

	S5.200.P	Precivia®	Single use
			Packaging
			Box of 25

FOR AVASTIN®₁

- For Avastin® injection*
- Compatible with insulin type cannulas & safety needles such as BD U-100 & B/Braun 30 Ga models

	S5.200.I	Precivia®	Single use
			Packaging
			Box of 25

PRECIVIA® PACK

- 1x Wrapping Sheet 75x75 cm
- 1x Perforated Drape 53x50 cm
- 1x Precivia® (S5.200.P)
- 3x Pro Ophta Sticks
- 5x Compresses 5x5 cm
- 1x 30 Ga 12 mm Cannula





	S5.300.P	Pack IVT 1	Single use
			Packaging
			Box of 25

1: Registered trade mark of Genentech Inc. 2: Registered trade mark of Bayer AG. *Please verify the medical use of Avastin® with your local authorities. Precivia® is a Class Is medical device indicated for intravitreal injections and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459. Precivia® Pack is a Class Ila medical device indicated for intravitreal injections. It is distributed by FCI S.A.S. and manufactured by M.E.D. Medical Products GmbH – Notified Body: DQS Medizinprodukte GmbH CE n°0297.

90° ADJUSTABLE LASER PROBES

Exclusive design

- Angle of curvature: pressure-controlled (from 0° to 90°)
- Safe probe removal: goes back in straight position when releasing the handle
- Compatible with most laser machines
- 50% stiffer than competition
- Short stroke for optimal control
- Low pressure needed to actuate the handle
- Ultra precise concentric laser spot
- Available in 23 Ga, 25 Ga
- Sterile, box of 10

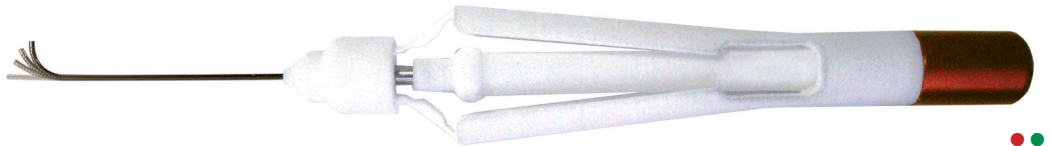

LASER CONNECTORS

ALCON® / COHERENT / ZEISS / ELLEX / OS4® / MERIDIAN AG / LIGHTMED

		Single use	23 Ga
S9.1302.23	90° Adjustable laser probe		
		Single use	25 Ga
S9.1302.25	90° Adjustable laser probe		



DORC

		Single use	23 Ga
S9.1305.23	90° Adjustable laser probe		
		Single use	25 Ga
S9.1305.25	90° Adjustable laser probe		



ENDO-PROBES

IRIDEX / BAUSCH+LOMB™

		Single use	23 Ga
S9.1301.23	90° Adjustable laser probe		
		Single use	25 Ga
S9.1301.25	90° Adjustable laser probe		



NIDEK THREAD

		Single use	23 Ga
S9.1304.23	90° Adjustable laser probe		
		Single use	25 Ga
S9.1304.25	90° Adjustable laser probe		



QUANTEL SUPRA® / VITRA®

		Single use	23 Ga
S9.1303.23	90° Adjustable laser probe		
		Single use	25 Ga
S9.1303.25	90° Adjustable laser probe		




DORC is a registered trade mark of D.O.R.C. Dutch Ophthalmic Research Center (International) B.V.; ALCON is a registered trade mark of NOVARTIS AG; COHERENT is a registered trade mark of COHERENT, Inc.; ZEISS is a registered trade mark of CARL ZEISS AG; ELLEX is a registered trade mark of Ellex Medical Pty Ltd; BAUSCH+LOMB™ is a registered trade mark of BAUSCH & LOMB™ Inc.; NIDEK is a registered trade mark of Nidek Co., Ltd.; QUANTEL is a registered trade mark of QUANTEL. The disposable 90° Adjustable laser probes are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

FCI DIRECTIONAL LASER PROBES


FCI DIRECTIONAL LASER PROBE

- Available in 23 Ga, 25 Ga
- Cursor-controlled angle: 0° to 90°
- Ultra precise concentric laser spot
- Compatible with most laser machines
- Sterile, box of 10

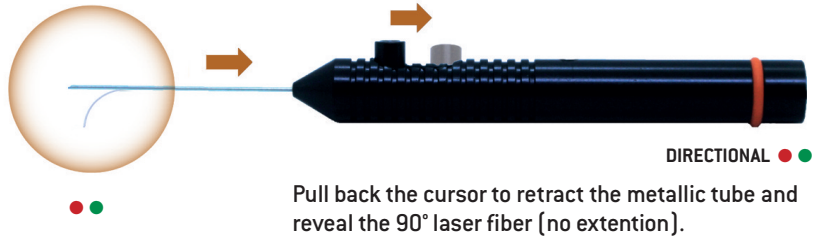

FCI DIRECTIONAL EXTENDABLE LASER PROBE

- Available in 23 Ga, 25 Ga
- Cursor-controlled angle: 0° to 90°
- Ultra precise concentric laser spot
- Compatible with most laser machines
- Sterile, box of 10

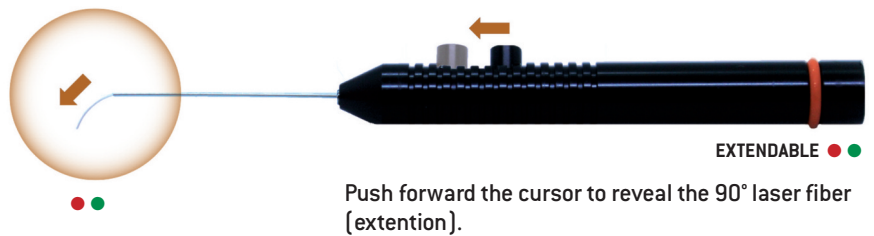

LASER CONNECTORS

ALCON® / COHERENT / ZEISS / ELLEX / OS4® / MERIDIAN AG / LIGHTMED

	Single use	23 Ga
S9.1312.23	FCI Directional laser probe	
S9.1322.23	FCI Directional extendable laser probe	

	Single use	25 Ga
S9.1312.25	FCI Directional laser probe	
S9.1322.25	FCI Directional extendable laser probe	



DORC

	Single use	23 Ga
S9.1315.23	FCI Directional laser probe	
S9.1325.23	FCI Directional extendable laser probe	

	Single use	25 Ga
S9.1315.25	FCI Directional laser probe	
S9.1325.25	FCI Directional extendable laser probe	



ENDO-PROBES

IRIDEX / BAUSCH+LOMB™

	Single use	23 Ga
S9.1311.23	FCI Directional laser probe	
S9.1321.23	FCI Directional extendable laser probe	

	Single use	25 Ga
S9.1311.25	FCI Directional laser probe	
S9.1321.25	FCI Directional extendable laser probe	



NIDEK THREAD

	Single use	23 Ga
S9.1314.23	FCI Directional laser probe	
S9.1324.23	FCI Directional extendable laser probe	

	Single use	25 Ga
S9.1314.25	FCI Directional laser probe	
S9.1324.25	FCI Directional extendable laser probe	



QUANTEL SUPRA® / VITRA®

	Single use	23 Ga
S9.1313.23	FCI Directional laser probe	
S9.1323.23	FCI Directional extendable laser probe	

	Single use	25 Ga
S9.1313.25	FCI Directional laser probe	
S9.1323.25	FCI Directional extendable laser probe	




DORC is a registered trade mark of D.O.R.C. Dutch Ophthalmic Research Center (International) B.V.; ALCON is a registered trade mark of NOVARTIS AG; COHERENT is a registered trade mark of COHERENT, Inc.; ZEISS is a registered trade mark of CARL ZEISS AG; ELLEX is a registered trade mark of Ellex Medical Pty Ltd; BAUSCH+LOMB™ is a registered trade mark of BAUSCH & LOMB™ Inc.; NIDEK is a registered trade mark of Nidek Co., Ltd.; QUANTEL is a registered trade mark of QUANTEL. The disposable FCI Directional laser probes are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

LASER PROBES

Ergonomic non-slip handpiece design

- Available in 20 Ga, 23 Ga, 25 Ga, 27 Ga
- Color coding for easy identification
- Ultra precise concentric laser spot
- Compatible with most laser machines
- Sterile, box of 10

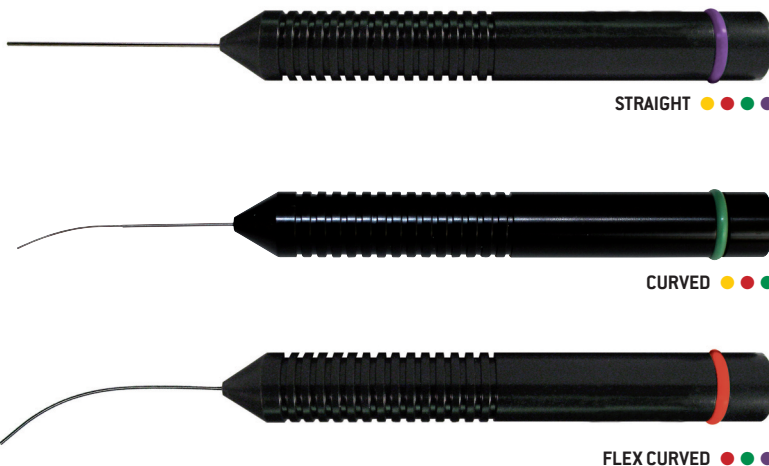

LASER CONNECTORS

ALCON® / COHERENT / ZEISS / ELLEX / OS4® / MERIDIAN AG / LIGHTMED

Single use		20 Ga
S9.1002.20	Straight	
S9.1102.20	Curved	

Single use		23 Ga
S9.1002.23	Straight	
S9.1202.23	Curved	
S9.1212.23	Flex curved	

Single use		25 Ga
S9.1002.25	Straight	
S9.1202.25	Curved	
S9.1212.25	Flex curved	

Single use		27 Ga
S9.1002.27	Straight	
S9.1212.27	Flex curved	



DORC

Single use		20 Ga
S9.1005.20	Straight	
S9.1105.20	Curved	

Single use		23 Ga
S9.1005.23	Straight	
S9.1205.23	Curved	
S9.1215.23	Flex curved	

Single use		25 Ga
S9.1005.25	Straight	
S9.1205.25	Curved	
S9.1215.25	Flex curved	

Single use		27 Ga
S9.1005.27	Straight	
S9.1215.27	Flex curved	



ENDO-PROBES

IRIDEX / BAUSCH+LOMB™

Single use		20 Ga
S9.1001.20	Straight	
S9.1101.20	Curved	

Single use		23 Ga
S9.1001.23	Straight	
S9.1201.23	Curved	
S9.1211.23	Flex curved	

Single use		25 Ga
S9.1001.25	Straight	
S9.1201.25	Curved	
S9.1211.25	Flex curved	

Single use		27 Ga
S9.1001.27	Straight	
S9.1211.27	Flex curved	



NIDEK THREAD

Single use		20 Ga
S9.1004.20	Straight	
S9.1104.20	Curved	

Single use		23 Ga
S9.1004.23	Straight	
S9.1204.23	Curved	
S9.1214.23	Flex curved	

Single use		25 Ga
S9.1004.25	Straight	
S9.1204.25	Curved	
S9.1214.25	Flex curved	

Single use		27 Ga
S9.1004.27	Straight	
S9.1214.27	Flex curved	



QUANTEL SUPRA® / VITRA®

Single use		20 Ga
S9.1003.20	Straight	
S9.1103.20	Curved	

Single use		23 Ga
S9.1003.23	Straight	
S9.1203.23	Curved	
S9.1213.23	Flex curved	

Single use		25 Ga
S9.1003.25	Straight	
S9.1203.25	Curved	
S9.1213.25	Flex curved	

Single use		27 Ga
S9.1003.27	Straight	
S9.1213.27	Flex curved	




DORC is a registered trade mark of D.O.R.C. Dutch Ophthalmic Research Center (International) B.V.; ALCON is a registered trade mark of NOVARTIS AG; COHERENT is a registered trade mark of COHERENT, Inc.; ZEISS is a registered trade mark of CARL ZEISS AG; ELLEX is a registered trade mark of Ellex Medical Pty Ltd; BAUSCH+LOMB™ is a registered trade mark of BAUSCH & LOMB™ Inc.; NIDEK is a registered trade mark of Nidek Co., Ltd.; QUANTEL is a registered trade mark of QUANTEL. The disposable laser probes are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

LASER ILLUMINATION PROBES

Ergonomic non-slip hanpiece design

- Available in 20 Ga, 23 Ga, 25 Ga, 27 Ga
- Color coding for easy identification
- Ultra precise concentric laser spot
- Compatible with most laser machines
- Sterile, box of 10

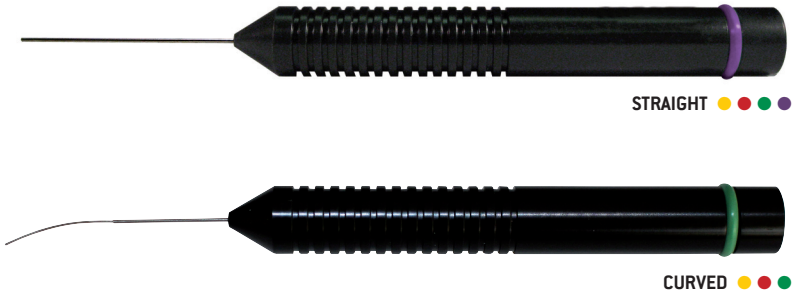

19 Ga needle

- Unique design with universal 19 Ga needle, to be inserted into FCI reusable light connector (page 14)



LASER CONNECTORS

ALCON® / COHERENT / ZEISS / ELLEX / OS4® / MERIDIAN AG / LIGHTMED

Single use		20 Ga
S9.1402.20	Straight	
S9.1502.20	Curved	

Single use		23 Ga
S9.1402.23	Straight	
S9.1602.23	Curved	

Single use		25 Ga
S9.1402.25	Straight	
S9.1602.25	Curved	

Single use		27 Ga
S9.1402.27	Straight	



DORC

Single use		20 Ga
S9.1405.20	Straight	
S9.1505.20	Curved	

Single use		23 Ga
S9.1405.23	Straight	
S9.1605.23	Curved	

Single use		25 Ga
S9.1405.25	Straight	
S9.1605.25	Curved	

Single use		27 Ga
S9.1405.27	Straight	



ENDO-PROBES

IRIDEX / BAUSCH+LOMB™

Single use		20 Ga
S9.1401.20	Straight	
S9.1501.20	Curved	

Single use		23 Ga
S9.1401.23	Straight	
S9.1601.23	Curved	

Single use		25 Ga
S9.1401.25	Straight	
S9.1601.25	Curved	

Single use		27 Ga
S9.1401.27	Straight	



NIDEK THREAD

Single use		20 Ga
S9.1404.20	Straight	
S9.1504.20	Curved	

Single use		23 Ga
S9.1404.23	Straight	
S9.1604.23	Curved	

Single use		25 Ga
S9.1404.25	Straight	
S9.1604.25	Curved	

Single use		27 Ga
S9.1404.27	Straight	



QUANTEL SUPRA® / VITRA®

Single use		20 Ga
S9.1403.20	Straight	
S9.1503.20	Curved	

Single use		23 Ga
S9.1403.23	Straight	
S9.1603.23	Curved	

Single use		25 Ga
S9.1403.25	Straight	
S9.1603.25	Curved	

Single use		27 Ga
S9.1403.27	Straight	



DORC is a registered trade mark of D.O.R.C. Dutch Ophthalmic Research Center (International) B.V.; ALCON is a registered trade mark of NOVARTIS AG; COHERENT is a registered trade mark of COHERENT, Inc.; ZEISS is a registered trade mark of CARL ZEISS AG; ELLEX is a registered trade mark of Ellex Medical Pty Ltd; BAUSCH+LOMB™ is a registered trade mark of BAUSCH & LOMB™ Inc.; NIDEK is a registered trade mark of Nidek Co., Ltd.; QUANTEL is a registered trade mark of QUANTEL. The disposable laser illumination probes (Class IIa) are medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

LIGHT CONNECTORS


FCI reusable light connectors are necessary for using Laser Illumination Probes and/or Light Probes.

FCI Laser Illumination Probes and Light Probes come with a 19 Ga universal needle, that has to be inserted into the reusable light connector. Once this is done, the connector is then plugged into the light source socket of the vitrectomy machine.

At the end of the procedure, the 19 Ga universal needle is removed from the reusable connector. This connector can stay connected to the light source, and will be used again for future surgeries by receiving another 19 Ga needle attached to a new disposable light probe.

- Reusable, box of 1
- Non sterile

S9.24.0A	Alcon Accurus® & Constellation®
S9.24.0B	Bausch+Lomb Millenium®
S9.24.0D	Bausch+Lomb Stellaris® PC
S9.24.0E	Dorc
S9.24.0F	Zeiss

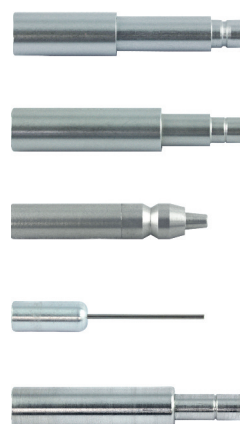

The reusable light connectors are Class I medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

ENDO-PROBES

LIGHT PROBES

Ergonomic non-slip handpiece design

- Convenient 2.4 meters long fibers
- Available in 20 Ga, 23 Ga, 25 Ga, 27 Ga
- Sterile, box of 10

19 Ga needle

- Unique design with universal 19 Ga needle, to be inserted into FCI reusable light connector (page 14)



Chandelier


- 360° illumination
- Silicone ring specifically designed to fit the trocar cannula and ensure both stability & sealing
- Safety magnet to avoid unexpected drop of the trocar cannula during procedure
- Silicone ring for chandelier depth adjustment
- Includes one trocar cannula mounted on ultra sharp knife
- Sterile, box of 10




Focus



Widefield

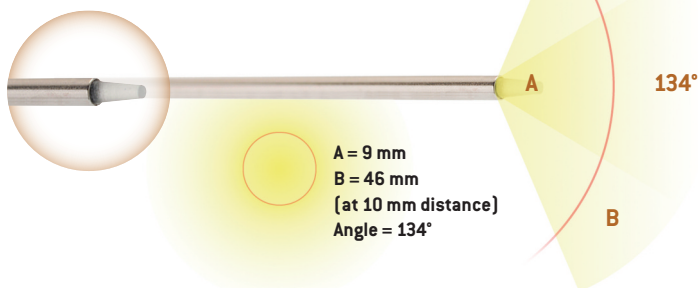

Shielded widefield

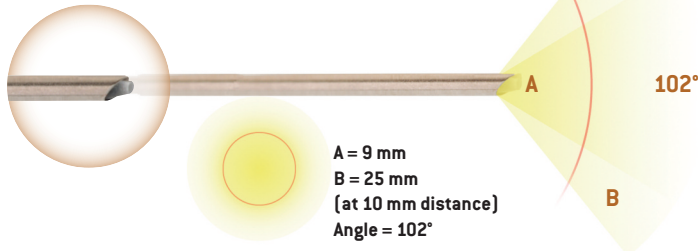

	Single use	20 Ga
S9.2001.20	Focus	
S9.2101.20	Widefield	
S9.2201.20	Shielded widefield	

	Single use	23 Ga
S9.2001.23	Focus	
S9.2101.23	Widefield	
S9.2201.23	Shielded widefield	

	Single use	25 Ga
S9.2001.25	Focus	
S9.2101.25	Widefield	
S9.2201.25	Shielded widefield	
S9.2301.25	Chandelier	

	Single use	27 Ga
S9.2001.27	Focus	

The disposable light probes are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

PURIFIED SILICONE OIL

FCI silicone oil is used for **prolonged tamponade** after a surgical treatment for severe retinal detachment.

- Highly purified
- Excellent stability
- Optimal transparency
- Exclusive vacuum molecular distillation & purification method
- 3-year shelf life
- Sterile, box of 1



VIAL



GLASS SYRINGE



	VISCOSITY	PACKAGING
S5.7180	1000 cSt	Vial 10 ml
S5.7100	1000 cSt	Vial 15 ml
S5.7580	5000 cSt	Vial 10 ml
S5.7500	5000 cSt	Vial 15 ml

	VISCOSITY	PACKAGING
S5.7170	1000 cSt	Syringe 10 ml
S5.7160	1000 cSt	Syringe 15 ml
S5.7570	5000 cSt	Syringe 10 ml
S5.7560	5000 cSt	Syringe 15 ml

RETIJET®

RetiJet® is FCI new silicone oil kit, with both injection and extraction functions.

For injection:

- One ready-to-use tubing system
- A green ring to secure FCI silicone oil syringe to the tubing set
- A choice of 23 Ga and 25 Ga injection cannulas

For extraction:

- One ready-to-use tubing system
- A green ring to secure the empty plastic syringe to the tubing set
- An extraction cannula
- Maximum pressure of 5 bars
- Sterile, box of 1



The purified silicone oil (Class IIb) and RetiJet® silicone oil kit (Class IIa) are medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

OPHTHALMIC SURGICAL LIQUIDS

Single use	INJECTION & EXTRACTION	MACHINES
	<p>S5.7591</p>	<p>Alcon: Accurus® - Constellation®</p> <p>Dorc: Eva®</p>
	<p>S5.7592</p>	<p>Bausch+Lomb: Millenium® - Stellaris® PC</p>
	<p>S5.7593</p>	<p>Oertli®: Orbit™ - Faros™ - OS3™ - OS4™</p> <p>Zeiss: Visalis 500 (for injection only)</p>
	<p>S5.7594</p>	<p>RUCK: PentaSys2, RUCK Qube® Pro</p> <p>Geuder: Megatron®, S3, S4, S4 HPS</p>

OPHTHALMIC SURGICAL LIQUIDS

PFCL

FCI-OCTA & FCI-DECA are liquids perfluorocarbons (PFCL) used in retinal surgery as a **transitory intra-ocular tamponade**, especially in retinal detachment.

- Perfectly pure
- Non volatile residues
- Non detectable fluorides
- Non detectable Ion hydrogen C-H link
- Supplied with sterile disposable needle & syringe
- 3-year shelf life
- Sterile, box of 1

		PACKAGING
S5.8150	FCI-DECA	Vial 5 ml
S5.8170	FCI-DECA	Vial 7 ml
S5.8250	FCI-OCTA	Vial 5 ml
S5.8270	FCI-OCTA	Vial 7 ml



S5.8150



S5.8170



S5.8250



S5.8270

The perfluorocarbons liquids are Class IIb medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

SCLERAL BUCKLES


ePTFE

Expanded PolyTetraFluoroEthylene (ePTFE) scleral buckles implants are porous and biocolonizable material. They are used to treat retinal detachment.

Main characteristics:

- Good conjunctival & scleral tolerance
- No inflammation
- No extrusion
- No conjunctival erosion
- No necrosis
- FCI exclusivity
- Sterile, box of 1

FCI EXCLUSIVE

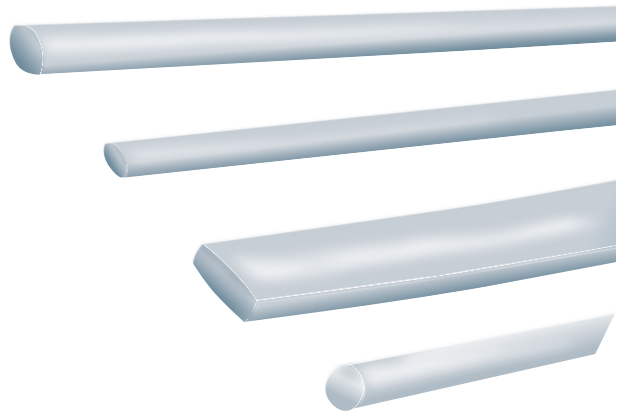

Bands

		Single use	LENGTH mm
S5.4801		Ducournau® Band	120
S5.4806		Ducournau® Band	60
S5.4811		Ducournau® Band	120

		Single use	LENGTH mm
S5.4821		Band	120
S5.8001		Band for reinforcing sclera at the back of the eye	120

Sponges

		Single use	LENGTH mm
S5.6625		Sponge	90
S5.6630		Sponge	90
S5.6635		Sponge	90
S5.6640		Sponge	90

		Single use	LENGTH mm
S5.6645		Half Sponge	90
S5.6650		Sponge	90
S5.6670		Sponge	90

Strips


		Single use	LENGTH mm
S5.6660		O. Lequoy® strip	90

SILICONE

FCI medical grade silicone implants for scleral buckling have been used in retinal detachment surgery throughout the world with excellent track record.

Main characteristics:

- Soft & elastic
- Biocompatible & non toxic
- Non-antigenic
- Easily tailored to exact size
- Wide range of shapes available
- Sterile

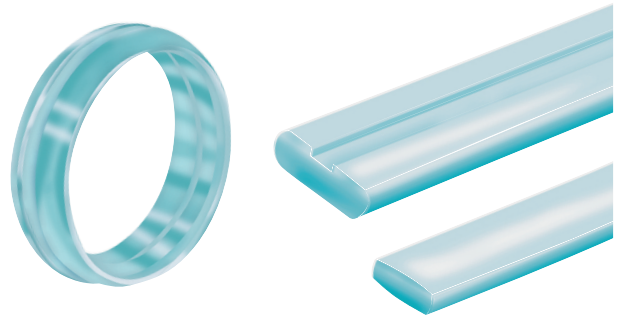

Bands *

		Single Use	LENGTH mm	BOX
S5.1000		Type 40	120	x 3
S5.1010		Type 41	120	x 3
S5.1020		Type 42	120	x 3
S5.2000		Type 240	120	x 3
S5.2010		Morin® band	100	x 3
S5.2282		Korobelnik® oval strip	120	x 1

		Single Use	LENGTH mm	BOX
S5.4000		Ducournau® band	120	x 3
S5.4100		Ducournau® band	120	x 3
S5.4200		Ducournau® band	120	x 3
S5.4300		Ducournau® band	120	x 3
S5.4450		Ducournau® band	120	x 3
S5.4500		Ducournau® band II	120	x 3

* Supplied with silicone fixation sleeve, except for Ducournau® bands

Ducournau® hooks

- Used to position silicone Ducournau® band II
- Non sterile, box of 1

S5.4900	Right Ducournau® hook
S5.4910	Left Ducournau® hook








The Ducournau® hooks (Class I) are indicated for vitreoretinal surgery and are manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.




SCLERAL BUCKLES




Strips

	Single Use	LENGTH mm	BOX
S5.1100	 Type 20	100	x 3
S5.1200	 Type 31	100	x 3
S5.1250	 Type 32	100	x 3
S5.2100	 Type 219	100	x 3
S5.2200	 Type 220	100	x 3



	Single Use	LENGTH mm	BOX
S5.2250	 Type 225	100	x 3
S5.1111	 Strip	100	x 1
S5.2261	 Morin® strip	100	x 1
S5.2271	 Caputo® zip strip 9 mm	120	x 1
S5.2276	 Caputo® zip strip 7 mm	120	x 1

Tires

	Single Use	BOX
S5.2290	 Asymmetrical tire Type 276	x 3
S5.2300	 Type 277	x 3
S5.2310	 Biconvex tire Type 287	x 3

	Single Use	BOX
S5.2320	 Biconvex tire Type 289	x 3
S5.2330	 Type 279	x 3
S5.2340	 Asymmetrical tire Type 280	x 3

Fixation sleeves


	Single Use	LENGTH mm	BOX
S5.3000	 Type 70 for S5.1000 / S5.1010	30	x 3
S5.3010	 Type 270 for S5.2000	30	x 3

	Single Use	LENGTH mm	BOX
S5.3020	 For S5.1020	30	x 3

Fixation sleeves forceps

- Non sterile, box of 1

S5.3100 Watzke forceps



S5.3100



Cords

		Single Use	LENGTH mm	BOX
S5.5110		Cord	150	x 3
S5.5115		Cord	150	x 3
S5.5120		Cord	150	x 3
S5.5020		Cord	150	x 1
S5.5130		Cord	150	x 3
S5.5030		Cord	150	x 1

		Single Use	LENGTH mm	BOX
S5.5150		Cord	150	x 3
S5.5050		Cord	150	x 1
S5.5330		Half cord	150	x 1
S5.5340		Half cord	150	x 1
S5.5350		Half cord	150	x 1

The fixation sleeves forceps (Class I) are indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

SCLERAL BUCKLES

Sponges

		Single Use	LENGTH mm	BOX
S5.6521		Type 501	100	x 1
S5.6303		Type 503	100	x 3
S5.6304		Type 504	100	x 3
S5.6305		Type 505	100	x 3
S5.6320		Type 505 G	100	x 3
S5.6335		Type 506	100	x 3
S5.6340		Type 506 G	100	x 3
S5.6357		Type 507	100	x 3
S5.6360		Type 507 G	100	x 3
S5.6311		Type 508	100	x 3
S5.6011				x 1
S5.6021		Type 508 G	100	x 1
S5.6370		Type 509 G	100	x 3

		Single Use	LENGTH mm	BOX
S5.6450		Type 510	100	x 3
S5.6150				x 1
S5.6475		Type 511	100	x 3
S5.6175				x 1
S5.6050		Oval	100	x 1
S5.6080		Sponge	100	x 1
S5.6160		Devin® half sponge	100	x 1
S5.6325		Furia® sponge	100	x 3
S5.6095		Gain® sponge	100	x 1
S5.6575		Korobelnik® coated sponge	10	x 1
S5.6535		Korobelnik® coated sponge	10	x 1
S5.6511		Sahel® sponge	100	x 1
S5.6531		Sahel® sponge	100	x 1
S5.6090		Trepsat® double radius sponge	100	x 1
S5.6085		Trepsat® oval sponge	100	x 1


The disposable scleral buckles (bands, sponges, strips, tires, cords) are Class IIb medical devices indicated for posterior segment surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

TROCARS

RetiLock® 1st one-step & autostable FCI trocar system


Main characteristics:

- Exclusive & patented design to ensure a good stability of the cannula, with special scleral ring feature
- Ready-to-use for a one-step insertion
- Ultra sharp knife for smooth & high precision incision
- Cone-shaped cannula to make the insertion of instruments easier
- 3 & 4 mm scleral marker
- Supplied with a 23 Ga / 25 Ga infusion line compatible with BSS, gas & silicone oil
- Sterile, box of 5 kits

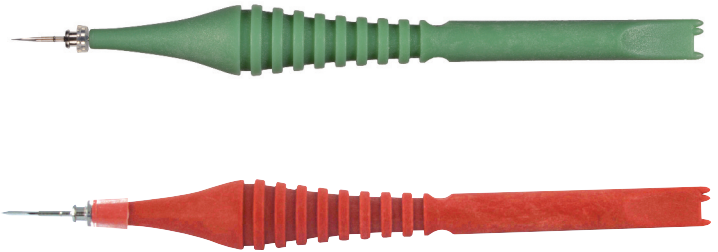

RetiLock® valved


- 3 Trocar cannulas mounted on ultra sharp knives
- 1 infusion line
- Transparent removable silicone valve and cone-shaped cannula for easy insertion of instruments

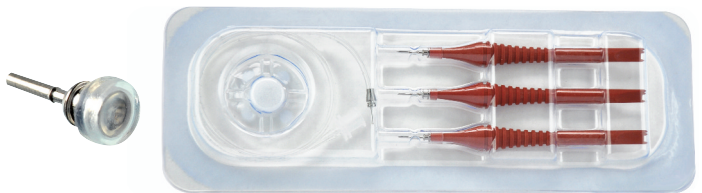

S9.7100 ●●

RetiLock® non valved

- 3 Trocar cannulas mounted on ultra sharp knives
- 1 infusion line
- Cone-shaped cannula for easy insertion of instruments
- 3 plugs: compatible with standard forceps such as Paufigue and Bonn forceps

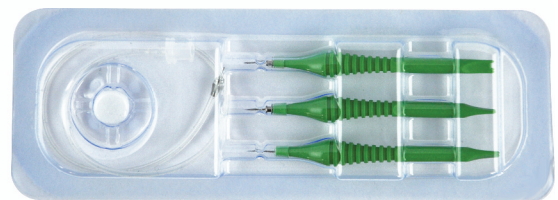

S9.7000 ●●

It is recommended to gently insert the plug on the trocar.

		Single use	23 Ga
S9.7000.23	Retilock® non valved		
S9.7100.23	Retilock® valved		
		Single use	25 Ga
S9.7000.25	Retilock® non valved		
S9.7100.25	Retilock® valved		


The disposable RetiLock® trocar systems are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

ACCESSORIES

DISPOSABLE BACKFLUSH WITH T-TUBE

Disposable backflush handpiece

- All-in-one & ready to use
- T-tube for easy insertion into the trocar cannula & protection of the tip
- Black silicone tips for better visibility
- Large reservoir for maximum reflux volume
- Plug for active / passive conversion
- Luer lock for active line attachment
- Male-Male luer lock included
- Available in 20 Ga, 23 Ga, 25 Ga, 27 Ga
- Sterile, box of 5

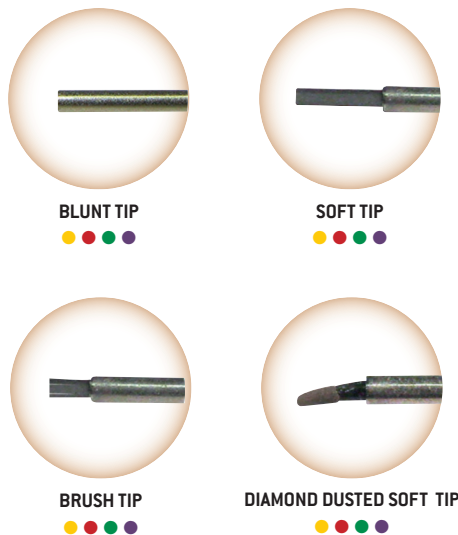

Single use		20 Ga
S9.3012.20	Blunt tip	
S9.3011.20	Brush tip with T-tube	
S9.3013.20	Diamond dusted soft tip with T-tube	
S9.3010.20	Soft tip with T-tube	

Single use		23 Ga
S9.3012.23	Blunt tip	
S9.3011.23	Brush tip with T-tube	
S9.3013.23	Diamond dusted soft tip with T-tube	
S9.3010.23	Soft tip with T-tube	

Single use		25 Ga
S9.3012.25	Blunt tip	
S9.3011.25	Brush tip with T-tube	
S9.3013.25	Diamond dusted soft tip with T-tube	
S9.3010.25	Soft tip with T-tube	

Single use		27 Ga
S9.3012.27	Blunt tip	
S9.3011.27	Brush tip with T-tube	
S9.3013.27	Diamond dusted soft tip with T-tube	
S9.3010.27	Soft tip with T-tube	

The disposable backflush handpieces are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

CANNULAS

Disposable cannulas

- Several tips design available
- T-tube for easy insertion into the trocar cannula & protection of the tip
- Black silicone tips for better visibility
- Sterile, box of 5

		Single use	20 Ga
S9.4112.20	Blunt tip		
S9.4111.20	Brush tip		
S9.4110.20	Soft tip		
		Single use	23 Ga
S9.4112.23	Blunt tip		
S9.4111.23	Brush tip with T-tube		
S9.4110.23	Soft tip with T-tube		
		Single use	25 Ga
S9.4112.25	Blunt tip		
S9.4111.25	Brush tip with T-tube		
S9.4110.25	Soft tip with T-tube		
		Single use	27 Ga
S9.4112.27	Blunt tip		
S9.4111.27	Brush tip with T-tube		
S9.4110.27	Soft tip with T-tube		

Dual bore cannulas






- Sterile, box of 5

		Single use	20 Ga
S9.4113.20	Dual bore cannula		
		Single use	23 Ga
S9.4113.23	Dual bore cannula		
		Single use	25 Ga
S9.4113.25	Dual bore cannula		

Sub-retinal cannulas

- 41 Ga tip
- Sterile, box of 5

		Single use	23 Ga
S9.4114.23	Sub-retinal cannula		
		Single use	25 Ga
S9.4014.25	Sub-retinal cannula		

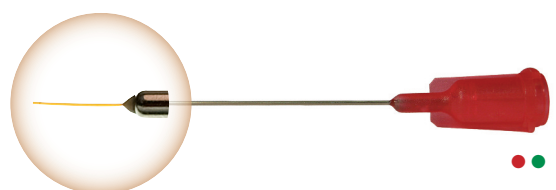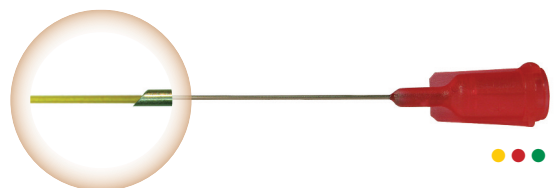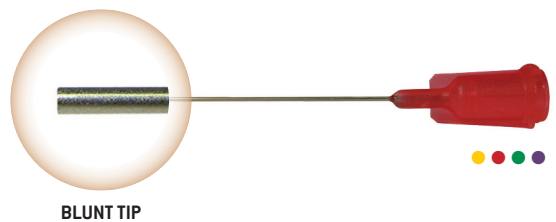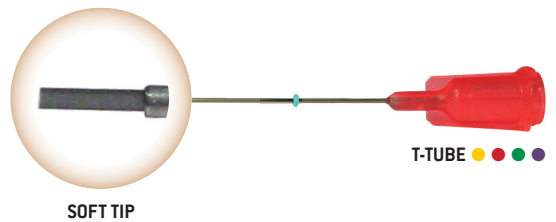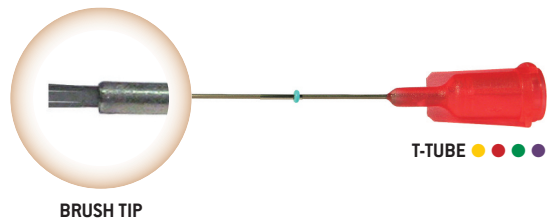

The disposable cannulas are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

ACCESSORIES

DISPOSABLE VITRECTOMY LENSES

Silicone vitrectomy lenses

- Sterile, box of 5

	Single use	FIELD	MAGNIFICATION	LANDERS RING COMPATIBILITY
S5.7010	Plano concave	30°	x 1.08	Yes
S5.7030	30° Prismatic	30°	x 1.08	Yes
S5.7040	Biconcave	36°	x 0.54	Yes



PLANO CONCAVE



PRISMATIC



BICONCAVE

PMMA vitrectomy lenses

- Sterile, box of 5

	Single use	FIELD	MAGNIFICATION	LANDERS RING COMPATIBILITY
S5.8010	Plano concave	30°	x 0.94	Yes
S5.8030	35° Prismatic	32°	x 0.94	Yes
S5.8040	Biconcave	31.8°	x 0.7	Yes



AUTOSTABLE PLANO CONCAVE

PMMA autostable plano concave lens

- Sterile, box of 5

	Single use	FIELD	MAGNIFICATION	LANDERS RING COMPATIBILITY
S5.8050	PMMA autostable plano concave	30°	x 0.94	N/A

FCI Protect® - 2.0% HPMC*

1st FCI Ophthalmic Viscosurgical Device (OVD)

- Volume substitute for aqueous humor during intraocular surgery
- Can be used as a contact gel with FCI disposable vitrectomy lenses
- Supplied with a sterile single use 23 Ga cannula
- Sterile, box of 10

	Single use
S5.9100	FCI Protect® 2.0 %



* HPMC: hydroxypropyl methylcellulose


The disposable vitrectomy lenses are Class Is medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459. FCI Protect® ophthalmic viscosurgical device is a Class IIb medical device indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

DISPOSABLE THREE MIRROR LENS

- Made of PMMA
- Angulation of 59°, 67°, 75°
- Central view 30°
- Image magnification 0.93x
- Sterile, box of 5



S5.8000

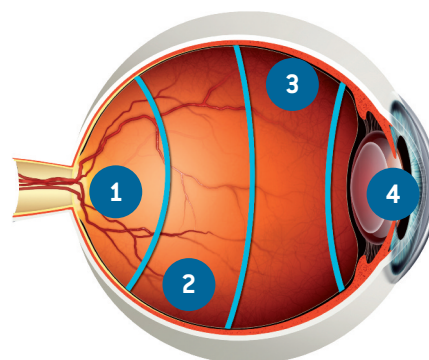

Single use

S5.8000

Disposable three mirror lens

Exceptional visualisation every time

Zone 1: Lens for observing the posterior pole up to 30°

Zone 2: 75° inclined mirror for observing the fundus above the 30° mark


Zone 3: 67° inclined mirror for observing the peripheral retina

Zone 4: 59° inclined mirror for observing the vitreous body and the aeras of the fundus alongside the ora serrata, as well as for gonioscopic examinations.

IRIS RETRACTORS

Single use iris retractors

- New design: flat bottom container covered with a transparent protective case to prevent the retractors from dropping.
- 5 hooks per set in upward position ready to pick up
- Folded adjustable silicone ring
- Nylon iris retractors
- Insertion through 0.5 mm incision
- Sterile

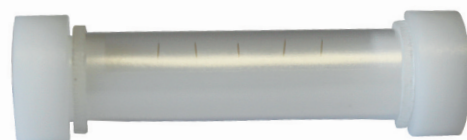

Single use

PACKAGING

S9.5054	Iris retractors - Disposable	5 pack of 5
S9.5015	Iris retractors - Disposable	1 pack of 5

The disposable three mirror lens is a Class Is medical device indicated for physical examination and vitreoretinal surgery, and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459. The disposable iris retractors are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.

ACCESSORIES

SINGLE USE INSTRUMENTS

SUPER GRIP FORCEPS

- Micro serrations on the broad platforms to grasp fibrous membranes
- 360° handle actuation
- Innovative « 3D » anti-shredding tips design with 100 grams grasping force
- Longer shafts for myopic eyes: 32 mm length
- Low pressure needed to actuate handle
- Short stroke for optimal control
- Color coding for easy identification
- Removable handle for selective dexterity
- Available in 23 Ga, 25 Ga, 27 Ga
- Sterile, box of 5



Single use 23 Ga
 S9.6018.23 Super Grip

Single use 25 Ga
 S9.6018.25 Super Grip

Single use 27 Ga
 S9.6018.27 Super Grip

VITREORETINAL INSTRUMENTS

SINGLE USE INSTRUMENTS

- Innovative anti-shredding tips design
- Maximum grasping power of 100 grams
- Low pressure needed to actuate the handle
- Short stroke for optimal control
- Exceptional precision: no forward / backward movement of the instrument tip
- Color coding for easy identification
- Available in 23 Ga, 25 Ga, 27 Ga
- Sterile, box of 5


FORCEPS




Single use		23 Ga
S9.6017.23	Tano	
S9.6011.23	Serrated	
S9.6012.23	Maculorhexis	
S9.6013.23	End-grasping	

Single use		25 Ga
S9.6017.25	Tano	
S9.6011.25	Serrated	
S9.6012.25	Maculorhexis	
S9.6013.25	End-grasping	


Single use		27 Ga
S9.6017.27	Tano	
S9.6012.27	Maculorhexis	
S9.6013.27	End-grasping	




TANO



SERRATED



MACULORHEXIS




END-GRASPING


SCISSORS



Single use		23 Ga
S9.6014.23	Horizontal	
S9.6015.23	Vertical	



HORIZONTAL



VERTICAL

Single use		25 Ga
S9.6014.25	Horizontal	
S9.6015.25	Vertical	


TANO POLISHER

- Color coding for easy identification
- Available in 20 Ga, 23 Ga, 25 Ga
- T-tube for easy insertion into the trocar cannula & protection of the tip
- Black diamonds and black silicone tip for better visibility
- Real diamond dust
- Sterile, box of 5



Single use		20 Ga
S9.6016.20	Tano polisher	

Single use		23 Ga
S9.6016.23	Tano polisher	



TANO POLISHER TIP

Single use		25 Ga
S9.6016.25	Tano polisher	

The disposable instruments are Class IIa medical devices indicated for vitreoretinal surgery and manufactured by FCI S.A.S. - Notified Body: GMED CE n°0459.



CONTACT INFORMATION

FCI S.A.S.

20/22 Rue Louis Armand
75015 Paris - FRANCE

Tél : +33 1 53 98 98 97

Fax : +33 1 53 98 98 99

fciworldwide@fci.fr




JOIN OUR OPHTHALMIC COMMUNITY!



LINKEDIN



YOUTUBE



EYETUBE



www.fciworldwide.com

FCI13/031.ind.E - June 2020 - Société par Actions Simplifiées au capital de 46 909 € - SIREN 351 670 385 - RCS PARIS. Conception : B.D.S.A. Le Havre - 02 35 19 21 16



For more information, please contact your local distributor :

Empty rounded rectangular box for distributor contact information.